

# World Journal of *Gastroenterology*

*World J Gastroenterol* 2018 August 21; 24(31): 3469-3566



**EDITORIAL**

- 3469 Locoregional therapy response in patients with hepatocellular cancer waiting for liver transplantation: Only selection or biological effect?

*Lai Q, Di Martino M, Lucatelli P, Mennini G*

**REVIEW**

- 3472 *Helicobacter pylori*: A foodborne pathogen?

*Quaglia NC, Dambrosio A*

- 3488 Hepatitis B virus infection: Defective surface antigen expression and pathogenesis

*Wu CC, Chen YS, Cao L, Chen XW, Lu MJ*

- 3500 Immunometabolism: A novel perspective of liver cancer microenvironment and its influence on tumor progression

*Zhang Q, Lou Y, Bai XL, Liang TB*

**MINIREVIEWS**

- 3513 Osteoporosis in primary biliary cholangitis

*Danford CJ, Trivedi HD, Papamichael K, Tapper EB, Bonder A*

- 3521 Ubiquitin-proteasome system and oxidative stress in liver transplantation

*Alva N, Panisello-Roselló A, Flores M, Roselló-Catafau J, Carbonell T*

**ORIGINAL ARTICLE****Basic Study**

- 3531 Stomach wall structure and vessels imaging by acoustic resolution photoacoustic microscopy

*Wang C, Lu YF, Cai CM, Xiang HZ, Zheng G*

- 3538 Clinical correlation of B7-H3 and B3GALT4 with the prognosis of colorectal cancer

*Zhang T, Wang F, Wu JY, Qiu ZC, Wang Y, Liu F, Ge XS, Qi XW, Mao Y, Hua D*

**Retrospective Cohort Study**

- 3547 Favorable clinical outcome of nonalcoholic liver cirrhosis patients with coronary artery disease: A population-based study

*Tsai MC, Yang TW, Wang CC, Wang YT, Sung WW, Tseng MH, Lin CC*

**Prospective Study**

- 3556 PillCamColon2 after incomplete colonoscopy - A prospective multicenter study

*Baltes P, Bota M, Albert J, Philipper M, Hörster HG, Hagenmüller F, Steinbrück I, Jakobs R, Bechtler M, Hartmann D, Neuhaus H, Charton JP, Mayershofer R, Hohn H, Rösch T, Groth S, Nowak T, Wohlmuth P, Keuchel M*

## Contents

*World Journal of Gastroenterology*  
Volume 24 Number 31 August 21, 2018

### ABOUT COVER

Editorial board member of *World Journal of Gastroenterology*, Tamara Vorobjova, DA, PhD, Academic Research, Department of Immunology, Institute of Biomedicine and Translational Medicine, University of Tartu, Tartu 51014, Estonia

### AIMS AND SCOPE

*World Journal of Gastroenterology* (*World J Gastroenterol*, *WJG*, print ISSN 1007-9327, online ISSN 2219-2840, DOI: 10.3748) is a peer-reviewed open access journal. *WJG* was established on October 1, 1995. It is published weekly on the 7<sup>th</sup>, 14<sup>th</sup>, 21<sup>st</sup>, and 28<sup>th</sup> each month. The *WJG* Editorial Board consists of 642 experts in gastroenterology and hepatology from 59 countries.

The primary task of *WJG* is to rapidly publish high-quality original articles, reviews, and commentaries in the fields of gastroenterology, hepatology, gastrointestinal endoscopy, gastrointestinal surgery, hepatobiliary surgery, gastrointestinal oncology, gastrointestinal radiation oncology, gastrointestinal imaging, gastrointestinal interventional therapy, gastrointestinal infectious diseases, gastrointestinal pharmacology, gastrointestinal pathophysiology, gastrointestinal pathology, evidence-based medicine in gastroenterology, pancreatology, gastrointestinal laboratory medicine, gastrointestinal molecular biology, gastrointestinal immunology, gastrointestinal microbiology, gastrointestinal genetics, gastrointestinal translational medicine, gastrointestinal diagnostics, and gastrointestinal therapeutics. *WJG* is dedicated to become an influential and prestigious journal in gastroenterology and hepatology, to promote the development of above disciplines, and to improve the diagnostic and therapeutic skill and expertise of clinicians.

### INDEXING/ABSTRACTING

*World Journal of Gastroenterology* (*WJG*) is now indexed in Current Contents<sup>®</sup>/Clinical Medicine, Science Citation Index Expanded (also known as SciSearch<sup>®</sup>), Journal Citation Reports<sup>®</sup>, Index Medicus, MEDLINE, PubMed, PubMed Central and Directory of Open Access Journals. The 2018 edition of Journal Citation Reports<sup>®</sup> cites the 2017 impact factor for *WJG* as 3.300 (5-year impact factor: 3.387), ranking *WJG* as 35<sup>th</sup> among 80 journals in gastroenterology and hepatology (quartile in category Q2).

### EDITORS FOR THIS ISSUE

Responsible Assistant Editor: *Xiang Li*  
Responsible Electronic Editor: *Yan Huang*  
Proofing Editor-in-Chief: *Lian-Sheng Ma*

Responsible Science Editor: *Xue-Jiao Wang*  
Proofing Editorial Office Director: *Ze-Mao Gong*

NAME OF JOURNAL  
*World Journal of Gastroenterology*

ISSN  
ISSN 1007-9327 (print)  
ISSN 2219-2840 (online)

LAUNCH DATE  
October 1, 1995

FREQUENCY  
Weekly

EDITORS-IN-CHIEF  
**Andrzej S Tarnawski, MD, PhD, DSc (Med),**  
**Professor of Medicine, Chief Gastroenterology, VA**  
Long Beach Health Care System, University of California, Irvine, CA, 5901 E. Seventh Str., Long Beach, CA 90822, United States

EDITORIAL BOARD MEMBERS  
All editorial board members resources online at <http://www.wjgnet.com/1007-9327/editorialboard.htm>

EDITORIAL OFFICE  
Ze-Mao Gong, Director  
*World Journal of Gastroenterology*  
Baishideng Publishing Group Inc  
7901 Stoneridge Drive, Suite 501,  
Pleasanton, CA 94588, USA  
Telephone: +1-925-2238242  
Fax: +1-925-2238243  
E-mail: [editorialoffice@wjgnet.com](mailto:editorialoffice@wjgnet.com)  
Help Desk: <http://www.f6publishing.com/helpdesk>  
<http://www.wjgnet.com>

PUBLISHER  
Baishideng Publishing Group Inc  
7901 Stoneridge Drive, Suite 501,  
Pleasanton, CA 94588, USA  
Telephone: +1-925-2238242  
Fax: +1-925-2238243  
E-mail: [bpgoffice@wjgnet.com](mailto:bpgoffice@wjgnet.com)  
Help Desk: <http://www.f6publishing.com/helpdesk>  
<http://www.wjgnet.com>

PUBLICATION DATE  
August 21, 2018

COPYRIGHT  
© 2018 Baishideng Publishing Group Inc. Articles published by this Open-Access journal are distributed under the terms of the Creative Commons Attribution Non-commercial License, which permits use, distribution, and reproduction in any medium, provided the original work is properly cited, the use is non commercial and is otherwise in compliance with the license.

SPECIAL STATEMENT  
All articles published in journals owned by the Baishideng Publishing Group (BPG) represent the views and opinions of their authors, and not the views, opinions or policies of the BPG, except where otherwise explicitly indicated.

INSTRUCTIONS TO AUTHORS  
Full instructions are available online at <http://www.wjgnet.com/bpg/gerinfo/204>

ONLINE SUBMISSION  
<http://www.f6publishing.com>

## Basic Study

# Stomach wall structure and vessels imaging by acoustic resolution photoacoustic microscopy

Cheng Wang, Yu-Fei Lu, Chun-Miao Cai, Hua-Zhong Xiang, Gang Zheng

Cheng Wang, Yu-Fei Lu, Hua-Zhong Xiang, Gang Zheng, Institute of Biomedical Optics and Optometry, School of Medical Instrument and Food Engineering, University of Shanghai for Science and Technology, Shanghai 200093, China

Chun-Miao Cai, Department of Pathology, Shanghai Tenth People's Hospital Affiliated to Tongji University, Shanghai 200093, China

ORCID number: Cheng Wang (0000-0002-6293-1607); Yu-Fei Lu (0000-0002-1446-0070); Chun-Miao Cai (0000-0003-3692-5120); Hua-Zhong Xiang (0000-0002-2544-4850); Gang Zheng (0000-0002-6818-0509).

**Author contributions:** Wang C designed and performed the research; Wang C and Lu YF wrote the paper; Cai CM harvested experimental samples and provided the pathology images; Wang C, Lu YF, Xiang HZ, and Gang Z performed the photoacoustic imaging experiment and processed the experiment data.

**Supported by the National Nature Science Foundation of China,** No. 61378060.

**Institutional review board statement:** This study was approved by the Laboratory Animal Ethics Committee of Shanghai Tenth People's Hospital. The design is reasonable and in line with the animal requirement. The ethics committee agreed to carry out a formal experiment.

**Conflict-of-interest statement:** To the best of our knowledge, no conflict of interest exists.

**Data sharing statement:** No additional data are available.

**Open-Access:** This article is an open-access article which was selected by an in-house editor and fully peer-reviewed by external reviewers. It is distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 4.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited and the use is non-commercial. See: <http://creativecommons.org/licenses/by-nc/4.0/>

Manuscript source: Unsolicited manuscript

**Correspondence to:** Cheng Wang, PhD, Associate Professor, Institute of Biomedical Optics and Optometry, School of Medical Instrument and Food Engineering, University of Shanghai for Science and Technology, No. 516 Jungong Road, Shanghai 200093, China. [c.wang@usst.edu.cn](mailto:c.wang@usst.edu.cn)  
Telephone: +86-21-55271165  
Fax: +86-21-55271200

Received: April 12, 2018

Peer-review started: April 13, 2018

First decision: May 17, 2018

Revised: May 26, 2018

Accepted: June 27, 2018

Article in press: June 27, 2018

Published online: August 21, 2018

## Abstract

### AIM

To image stomach wall blood vessels and tissue, layer-by-layer.

### METHODS

We built up the acoustic resolution photoacoustic microscopy (AR-PAM) system for imaging layered tissues, such as the stomach wall. A tunable dye laser system was coupled to a fiber bundle. The fibers of the bundle were placed in nine directions with an incident angle of 45° around a high-frequency ultrasound transducer attached to the acoustic lens. This structure formed a dark field on the tissue surface under the acoustic lens and the nine light beams from the fibers to be combined near the focal point of the acoustic lens. The sample piece was cut from a part of the porcine stomach into a petri dish. In order to realize photoacoustic depth imaging of tumor, we designed a tumor model based on indocyanine green (ICG) dye. The ICG solution (concentration of 129 μM/mL)



was mixed into molten gel, and then a gel mixture of ICG (concentration of 12.9  $\mu\text{M}/\text{mL}$ ) was injected into the stomach submucosa. The injection quantity was controlled by 0.1 mL to make a small tumor model.

## RESULTS

An acoustic resolution photoacoustic microscopy based on fiber illumination was established and an axial resolution of 25  $\mu\text{m}$  and a lateral resolution of 50  $\mu\text{m}$  in its focal zone range of 500  $\mu\text{m}$  has been accomplished. We tuned the laser wavelength to 600 nm. The photoacoustic probe was driven to do B-scan imaging in tissue thickness of 200  $\mu\text{m}$ . The photoacoustic micro-image of mucosa and submucosa of the tissue have been obtained and compared with a pathological photograph of the tissue stained by hematoxylin-eosin staining. We have observed more detailed internal structure of the tissue. We also utilized this photoacoustic microscopy to image blood vessels inside the submucosa. High contrast imaging of the submucosa tumor model was obtained using ICG dye.

## CONCLUSION

This AR-PAM is able to image layer-by-layer construction and some blood vessels under mucosa in the stomach wall without any contrast agents.

**Key words:** Photoacoustic imaging; Stomach; Layered tissue; Acoustic resolution; Fiber

© The Author(s) 2018. Published by Baishideng Publishing Group Inc. All rights reserved.

**Core tip:** In order to image layered tissue and blood vessels, acoustic resolution photoacoustic microscopy based on fiber illumination was established and an axial resolution of 25  $\mu\text{m}$  and a lateral resolution of 50  $\mu\text{m}$  in its focal zone range of 500  $\mu\text{m}$  was accomplished. Layer-by-layer imaging of the stomach tissue and stomach mucosa blood vessels were obtained. High contrast imaging of the submucosa tumor model was obtained using ICG dye.

Wang C, Lu YF, Cai CM, Xiang HZ, Zheng G. Stomach wall structure and vessels imaging by acoustic resolution photoacoustic microscopy. *World J Gastroenterol* 2018; 24(31): 3531-3537 Available from: URL: <http://www.wjgnet.com/1007-9327/full/v24/i31/3531.htm> DOI: <http://dx.doi.org/10.3748/wjg.v24.i31.3531>

## INTRODUCTION

Stomach submucosal tumors (SMT) are any intramural growth underneath the mucosa of the gastrointestinal tract<sup>[1]</sup>. These tumors are very hard to find because they are usually asymptomatic and therefore most often discovered as accidental findings during surgery, autopsy, and so on. When examining submucosal


tumors, standard optical stomach endoscopy, capsule optical endoscopy and push-and-pull enteroscopy together with barium contrast X-ray do not alone provide sufficient information. Endoscopic ultrasound (EUS), computed tomography (CT) and magnetic resonance imaging (MRI) are recommended as supplementary tools<sup>[2]</sup> because CT and MRI often lack either sufficient spatial resolution or satisfactory contrast (or both) to be effective for early-stage tumor imaging<sup>[3]</sup>. Optimal EUS imaging of an SMT needs submersion of the tumor under water. However, benign SMTs, for example the submucosal inflammation, cannot be distinguished endosonographically<sup>[4]</sup>. Therefore, early-phase tumor detection or in situ characterization of diseased tissue is challenging for EUS. Because the mechanism of EUS imaging is ultrasound imaging, this is based on tissue bulk mechanical properties. Tumor tissue boundaries and blood vessel structures are clinically relevant and provide necessary information for assessing disease stage and planning treatment therapies.

Recently, optical endoscopic imaging modalities, like narrow band imaging endoscopy<sup>[5]</sup>, endoscopic optical coherent tomography<sup>[6]</sup> and confocal laser endomicroscopy<sup>[7]</sup> have been developed. They can detect tissue or tissue changes with high sensitivity and high spatial resolution. Because of the strong optical scattering properties of tissue, these techniques are unable to image targets beyond a 1-2 mm depth. Photoacoustic imaging has a lot of advantages, such as, endogenous optical chromophore contrast enables label-free imaging of the microvasculature with a high resolution<sup>[8]</sup>, and *in vivo* blood vessel photoacoustic imaging can cover the length scale from a superficial capillary<sup>[9]</sup> to an abdominal aorta<sup>[10]</sup>, demonstrating the potential of photoacoustic imaging to bridge the resolution and penetration gaps between microvascular microscopy, clinical angiography and so on<sup>[11,12]</sup>. This paper's aim is to demonstrate that photoacoustic imaging is able to image the layered tissue and blood vessels under the surface of the tissue. In the future, we can design and develop an photoacoustic endoscopic imaging system to image deeper tissue with higher resolution for diagnosis and treatment.

## MATERIALS AND METHODS

### AR-PAM system

The acoustic resolution photoacoustic microscopy (AR-PAM) system for stomach wall imaging was shown in Figure 1A. A tunable dye laser system pumped by a Q-switch Nd:YAG laser (ND6000, continuum) was used to provide laser pulse with a pulse repetition of 10 Hz and a pulse width of 5.5 ns. The tunable range of the laser light was 415 nm to 940 nm. A pair of concave and convex lenses expanded and collimated the light beam to approximately 5 mm in diameter. Then coupling to a fiber bundle that was composed by nine optical fibers (FT400UMT, Thorlabs) which have a 400  $\mu\text{m}$  core

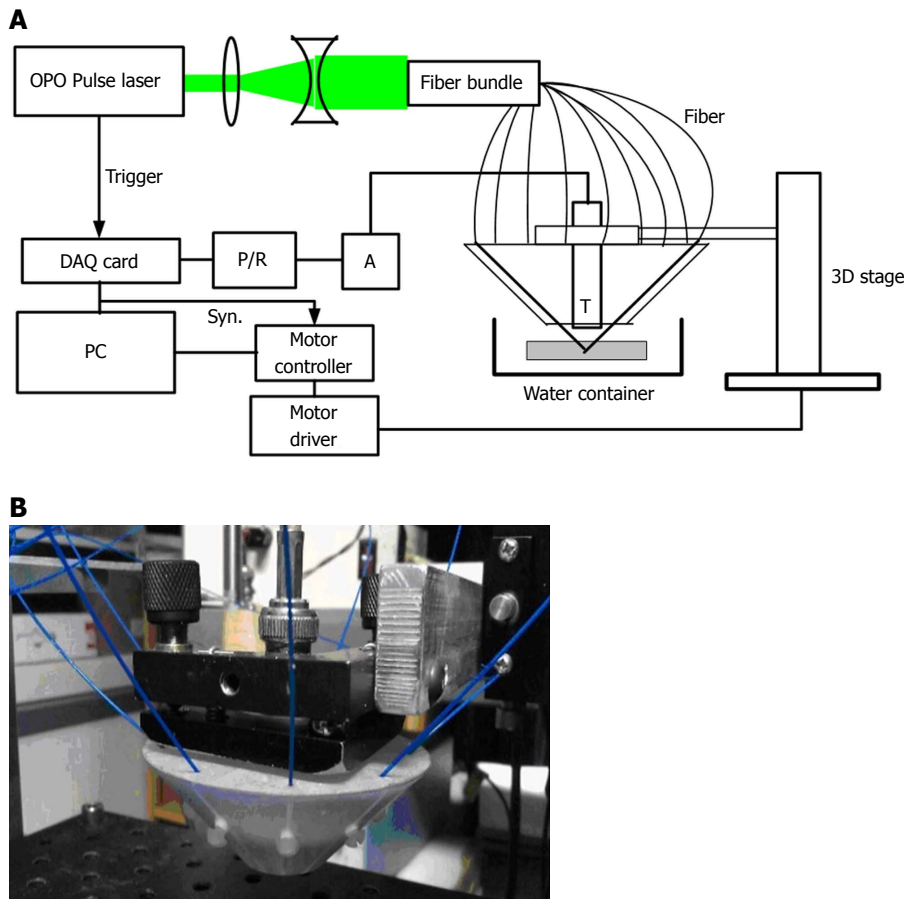

**Figure 1** Schematic of the acoustic resolution photoacoustic microscopy system (A) and photograph of the photoacoustic probe (B). P/R: Pulser/receiver; A: Preamplifier; T: Transducer, PC: Personal computer.

diameter and numerical aperture of 0.39 were placed in nine directions ( $40^\circ$  intervals in  $360^\circ$ ) around a high-frequency (50-MHz, bandwidth of 30 MHz) ultrasound transducer attached with the acoustic lens (the  $f/\#$  is 1.3 and focal length is 4 mm). The cross angle between the fibers with the transducer axis direction were set to  $45^\circ$ , so that it formed a dark field on the tissue surface under the acoustic lens and the nine light beams from the fibers were combined near the focal point of the acoustic lens, *i.e.* it is then weakly focused into the tissue with the focal region coaxially overlapping the ultrasonic focus inside the tissue. In an optically transparent medium, the optical focus is about 2 mm in diameter, which is much wider than the ultrasonic focus. The focal acoustic transducer and output end of the fibers were fastened with a holder made by a 3D printer. We can refer to it as a photoacoustic probe (Figure 1B). According to the parameters of the ultrasonic transducer, an axial resolution of  $25\ \mu\text{m}$  and a lateral resolution of  $50\ \mu\text{m}$  in its focal zone range of  $500\ \mu\text{m}$  can be accomplished. The photoacoustic probe is translated in a water bath. A window at the bottom of the water container is sealed with an optically and ultrasonically transparent disposable polyethylene membrane (thickness: 0.04 mm). After commercial ultrasound gel is applied to the region of interest on the sample for acoustic coupling, the sample is placed between the sample supporter and

the water container for imaging. The photoacoustic wave is recorded at each location of the ultrasonic transducer and subsequently converted into a one-dimensional (1D) depth-resolved image (A-scan) based on the sound velocity in soft tissue ( $1.54\ \text{mm}/\text{us}$ ). Images were generated by one dimension (B-Scan) in the X or Y direction or two-dimensional (C-Scan) raster scanning of the photoacoustic probe in the X-Y plane with a step size of  $30\ \mu\text{m}$ . In addition to, we can also scan in the Z direction with a step of  $200\ \mu\text{m}$  for producing an image of the deeper tissue by utilizing deeply penetrable diffused light to excite photoacoustic signals. At each scanning position, signals were recorded by an 8 bits digitizer card (DP1400, Agilent Tech, United States) after it was amplified by a preamplifier (AU-2A-0150-BNC, MTEQ, United States) and then amplified and filtered (high pass 1 MHz) by a pulser/receiver (5073PR, Olympus, Japan). No signal averaging is performed. As shown in Figure 2, photoacoustic imaging of a hair with a diameter of  $80\ \mu\text{m}$  were obtained with this photoacoustic system for verifying the imaging ability. Figure 2A was a B-scan image and Figure 2B was a C-scan image of the hair.

#### **Preparing a porcine stomach wall sample**

A porcine stomach was received the day after the animal was sacrificed for an unrelated study. The sample piece was cut from a part of the porcine stomach into a petri

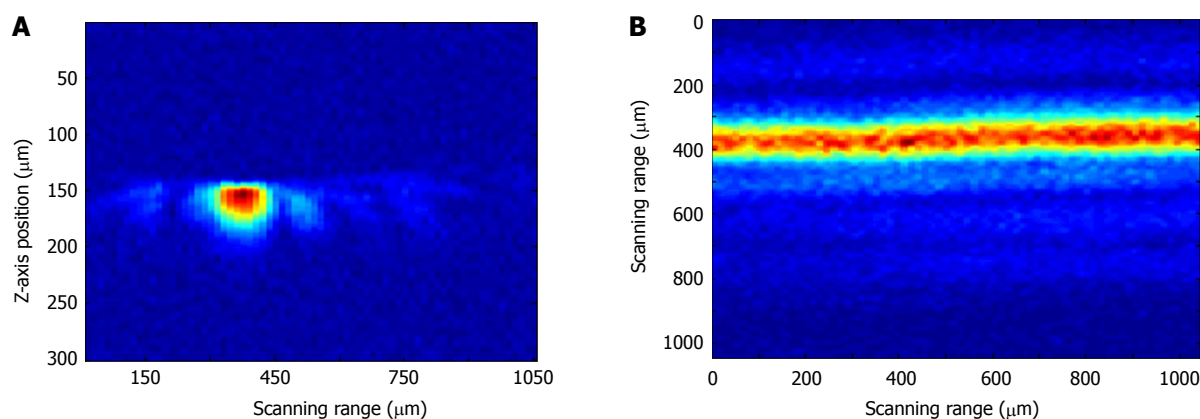


Figure 2 Photoacoustic image of a hair with a diameter of 80  $\mu\text{m}$ . A: B-scan imaging. B: C-scan imaging.

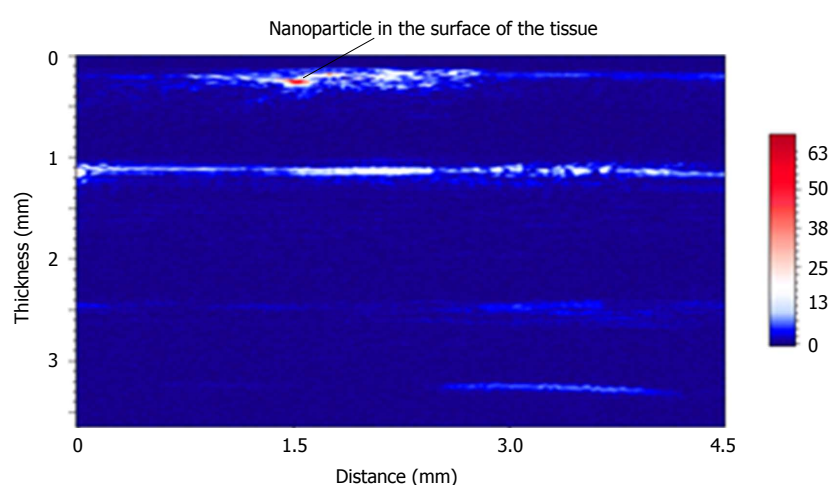


Figure 3 Imaging of layer-by-layer structure of stomach wall.

dish with a diameter of 140 mm and a thickness of 22 mm. In order to obtain a photoacoustic depth image of the tumor, we designed a tumor model based on indocyanine green (ICG) dye, wherein the ICG solution at a concentration of 129  $\mu\text{M}/\text{mL}$  was mixed into molten gel, and then the gel mixture of ICG at a concentration of 12.9  $\mu\text{M}/\text{mL}$  was injected into the stomach submucosa at a 2-3 mm position. The injection quantity was controlled to 0.1 mL to make a small tumor model.

## RESULTS

In order to verify photoacoustic imaging can also be used to implement stratified imaging of the stomach wall, we tuned the laser wavelength to 600 nm. The photoacoustic probe obtained many B-scan images at tissue thickness direction with a lateral scanning step of 200  $\mu\text{m}$ . Then, all of the B-scan images were combined to complete an image of the layered structure of the stomach wall (Figure 3). A particle with the diameter of 300  $\mu\text{m}$  was placed on the surface of stomach tissue, in order to indicate the surface position of the tissue. As shown in Figure 4, the photoacoustic microimage of the mucosa and submucosa of the tissue have been obtained

and compared with a pathological photograph of the tissue stained by hematoxylin-eosin staining. We have observed more detailed internal structure of the tissue by the photoacoustic imaging.

In addition, we also utilized this photoacoustic microscopy to image blood vessels inside the submucosa. The dissected stomach wall after imaging by photoacoustic microscopy is shown in Figure 5A. The vessels under submucosa after imaging by photoacoustic microscopy is shown in Figure 5B. We very clearly saw the artery vessels and vein vessels.

In order to realize the photoacoustic depth imaging of the tumor, we designed a labeled tumor model based on ICG dye, wherein 0.1 mL ICG gelatin solution with a concentration of 129  $\mu\text{M}/\text{mL}$  was injected into the stomach submucosa at 2-3 mm deep. After the ICG-gel mixture was injected into the tissue and coagulated for 20 minutes, the C-scan imaging at different depths was completed. When doing the scanning, the output wavelength of the laser was tuned to 700 nm because is the absorption peak of the ICG dye with molar extinction coefficient of  $1.1 \times 10^5 \text{ cm}^{-1}/\text{M}$  in water. This will improve the signal: noise ratio of the image.

Some diffusion phenomena of the ICG resolution



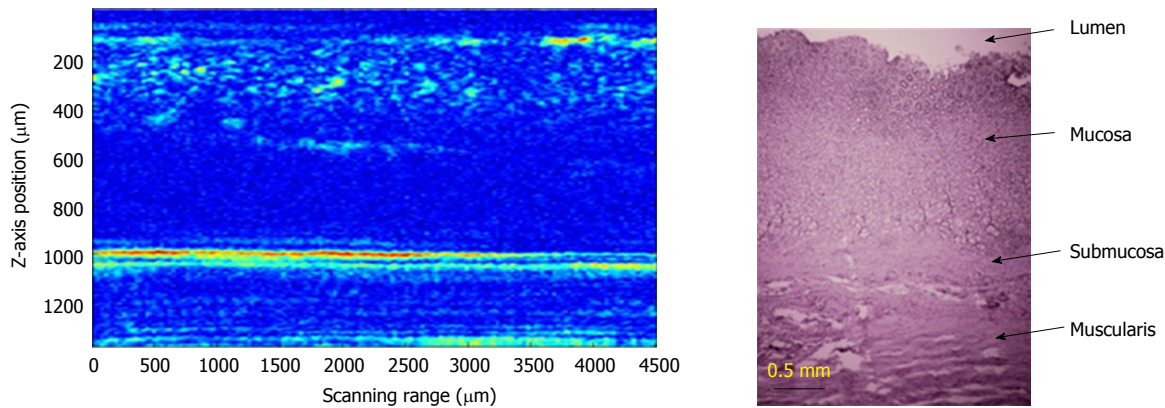


Figure 4 Compared photoacoustic image with pathological photograph stained by hematoxylin-eosin staining for mucosa and submucosa of the tissue.

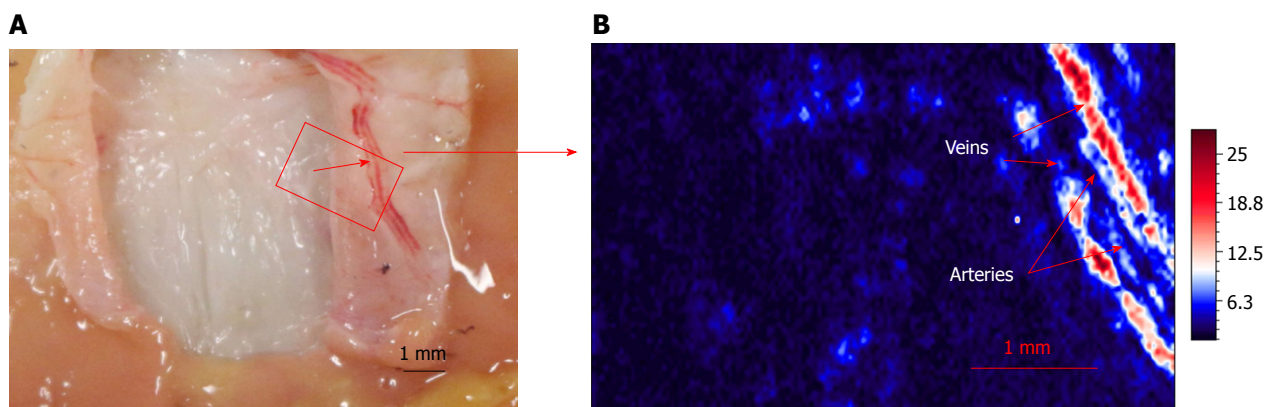


Figure 5 Photograph of the dissected stomach wall after imaging by photoacoustic microscopy (A) and photoacoustic imaging under surface of the tissue of 500 μm (red arrow indicate vessels) (B).

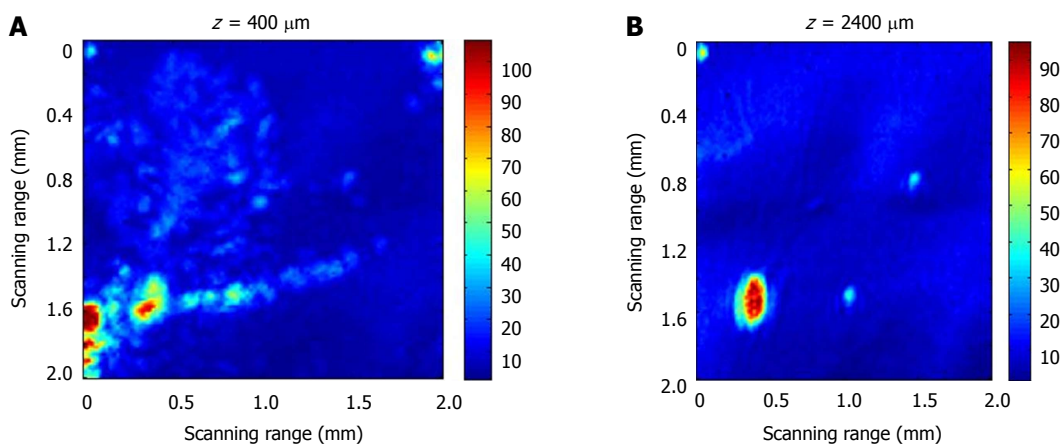


Figure 6 Photoacoustic imaging with laser wavelength of 700 nm for contrast agent with concentration of 12.9 μM/mL in depth of 400 μm (A) and 2400 μm (B).

at the mucosal site of 400 μm was observed (Figure 6A). The ICG dye may have combined with blood in the vessels, so some tubular structures were observed. At a depth of 2400 μm, the ICG labeled tumor model was still visible (Figure 6B). This indicated that we can achieve deeper detection.

## DISCUSSION

Ultrasound uses high-frequency sound waves to produce

images of the organs and structures inside the body such as ovaries, uterus, liver, gallbladder, pancreas, or aorta. EUS combines endoscopy and ultrasound in order to obtain images and information about the digestive tract and the surrounding tissue and organs. EUS can obtain information about the layers of the intestinal wall as well as adjacent areas such as lymph nodes and the blood vessels. EUS provides doctors with more information than other imaging tests by providing detailed images of the digestive tract. Although contrast-enhanced



ultrasonic techniques<sup>[13,14]</sup> such as Doppler ultrasound<sup>[15]</sup> are able to image blood vessels, the resolution of these imaging techniques are much lower than that of PAM, which has recently achieved lateral resolution up to 15  $\mu\text{m}$ <sup>[16]</sup>. Additionally, photoacoustic imaging provides functional information with endogenous contrast and with the aid of an exogenous contrast agent. Therefore, photoacoustic endoscopy based on photoacoustic tomography and EUS, which has achieved spatially coincident photoacoustic and ultrasonic imaging, provides unprecedented information and promotes morphologic and functional understanding of the gastrointestinal tract imaging<sup>[17]</sup>. But the research on tissue structure based on photoacoustic imaging technique has not been published yet. This paper reported that utilizing AR-PAM to image layered tissue in the stomach wall and blood vessels under the mucosa in s without any contrasting agents. In the next step, this acoustic resolution photoacoustic microscopy will combine with endoscopy and minimize the photoacoustic probe to make a micro-photoacoustic endoscopy for obtaining morphologic and functional information with higher resolution and depth *in vivo*.

In conclusion, we have presented a fiber illumination based acoustic resolution photoacoustic microscopy method. We have realized an axial resolution of 25  $\mu\text{m}$  and a lateral resolution of 50  $\mu\text{m}$  in its focal zone range of 500  $\mu\text{m}$ . This system was utilized to image layered stomach wall tissue and blood vessels under the mucosa without any contrasting agents. Using ICG dye enhance a tumor model, the tumor model was imaged to depths of 2400  $\mu\text{m}$  with very high contrast. The photoacoustic microscopy has the ability to image layered tissue with high resolution and high contrast.

## ARTICLE HIGHLIGHTS

### Research background

When checking submucosal tumors, traditional methods (such as standard optical stomach endoscopy, capsule optical endoscopy and push-and-pull enteroscopy together with barium contrast X-ray) can't provide accurate information. Computed tomography and magnetic resonance imaging are often lower in resolution and contrast. Optimal endoscopic ultrasound (EUS) imaging of stomach submucosal tumors (SMT) needs submersion of the tumor under water. However, benign SMTs, for example the submucosal inflammation, cannot be distinguished endosonographically. Therefore, it is still a challenge for EUS to detect early-phase tumor *in situ*. Our team aimed to demonstrate that photoacoustic imaging is able to image layered tissue and blood vessels under the surface of the tissue. In the future, we can design and develop a photoacoustic endoscopic imaging system to image deeper tissues with higher resolution for diagnosis and treatment.

### Research motivation

To image layered tissue and blood vessels in layered tissue.

### Research objectives

Our aim is to demonstrate that photoacoustic imaging can detect the structure of layered tissue and blood vessels beneath the surface of the tissue.

### Research methods

Our team established the acoustic resolution photoacoustic microscopy (AR-PAM) system for stomach wall structure imaging. Photoacoustic microimaging

of the stomach wall structure was compared to an HE pathology image to verify the structure, vessels, and vessel direction.

## Research results

As a result, we have established a fiber illumination based acoustic resolution photoacoustic microscopy method. The imaging ability has an axial resolution of 25  $\mu\text{m}$  and a lateral resolution of 50  $\mu\text{m}$  in its focal zone range of 500  $\mu\text{m}$ . We have observed more detailed internal structure of the tissue from AR-PAM imaging. We also utilized this photoacoustic microscopy to image blood vessels inside the submucosa. By using ICG dye enhance a tumor model in the submucosa, the images obtained at a depth of 2400  $\mu\text{m}$  depth had very high contrast.

## Research conclusions

In this study, we have established a fiber illumination based acoustic resolution photoacoustic microscopy. Layer-by-layer imaging of the stomach tissue and blood vessels under stomach mucosa were obtained. By using ICG dye to enhance the tumor model, high contrast images at a depth of 2400  $\mu\text{m}$  tissue were obtained. This proved that photoacoustic microscopy has the ability to image layered tissue and deep tissue targets with high resolution and high contrast. In the near future, this technique combined with endoscopy will supply a simple tool for physicians to see differences in layered tissues and imaging of tumor angiogenesis in submucosa.

## Research perspectives

This technique combined with endoscopy will supply a simple tool to visualize layered tissues and tumor angiogenesis in submucosa. Scientific research should aim at solving practical problems in clinical practice. Innovative scientific research is demonstrated in the ability to effectively solve the difficult problems doctors encounter in clinical practice.

## REFERENCES

- 1 **Chak A.** EUS in submucosal tumors. *Gastrointest Endosc* 2002; **56**: S43-S48 [PMID: 12297748 DOI: 10.1016/S0016-5107(02)70085-0]
- 2 **Hsu CC,** Chen JJ, Changchien CS. Endoscopic features of metastatic tumors in the upper gastrointestinal tract. *Endoscopy* 1996; **28**: 249-253 [PMID: 8739742 DOI: 10.1055/s-2007-1005437]
- 3 **Hu S,** Wang LV. Photoacoustic imaging and characterization of the microvasculature. *J Biomed Opt* 2010; **15**: 011101 [PMID: 20210427 DOI: 10.1117/1.3281673]
- 4 **Shim CS,** Jung IS. Endoscopic removal of submucosal tumors: preprocedure diagnosis, technical options, and results. *Endoscopy* 2005; **37**: 646-654 [PMID: 16010609 DOI: 10.1055/s-2005-861477]
- 5 **Han S,** Hsu A, Wassef WY. An update in the endoscopic management of gastric cancer. *Curr Opin Gastroenterol* 2016; **32**: 492-500 [PMID: 27662061 DOI: 10.1097/MOG.0000000000000318]
- 6 **Ding Z,** Qiu J, Shen Y, Chen Z, Bao W. Lens-free all-fiber probe with an optimized output beam for optical coherence tomography. *Opt Lett* 2017; **42**: 2814-2817 [PMID: 28708176 DOI: 10.1364/OL.42.002814]
- 7 **Karia K,** Kahaleh M. A Review of Probe-Based Confocal Laser Endomicroscopy for Pancreaticobiliary Disease. *Clin Endosc* 2016; **49**: 462-466 [PMID: 27642847 DOI: 10.5946/ce.2016.086]
- 8 **Zhang HF,** Maslov K, Stoica G, Wang LV. Functional photoacoustic microscopy for high-resolution and noninvasive in vivo imaging. *Nat Biotechnol* 2006; **24**: 848-851 [PMID: 16823374 DOI: 10.1038/nbt1220]
- 9 **Maslov K,** Zhang HF, Hu S, Wang LV. Optical-resolution photoacoustic microscopy for in vivo imaging of single capillaries. *Opt Lett* 2008; **33**: 929-931 [PMID: 18451942 DOI: 10.1364/OL.33.000929]
- 10 **Brecht HP,** Su R, Fronheiser M, Ermilov SA, Conjusteau A, Liopo A, Motamedi M, Oraevsky AA. Photoacoustic 3D whole-body tomography: experiments in nude mice. *Proc SPIE* 2009; **7177**: 71770E [DOI: 10.1117/12.812319]
- 11 **Wang X,** Xie X, Ku G, Wang LV, Stoica G. Noninvasive imaging

- of hemoglobin concentration and oxygenation in the rat brain using high-resolution photoacoustic tomography. *J Biomed Opt* 2006; **11**: 024015 [PMID: 16674205 DOI: 10.1117/1.2192804]
- 12 **Wang Y**, Hu S, Maslov K, Zhang Y, Xia Y, Wang LV. In vivo integrated photoacoustic and confocal microscopy of hemoglobin oxygen saturation and oxygen partial pressure. *Opt Lett* 2011; **36**: 1029-1031 [PMID: 21478972 DOI: 10.1364/OL.36.001029]
  - 13 **Ignée A**, Jenssen C, Hocke M, Dong Y, Wang WP, Cui XW, Woenckhaus M, Iordache S, Saftoiu A, Schuessler G, Dietrich CF. Contrast-enhanced (endoscopic) ultrasound and endoscopic ultrasound elastography in gastrointestinal stromal tumors. *Endosc Ultrasound* 2017; **6**: 55-60 [PMID: 28218202 DOI: 10.4103/2303-9027.200216]
  - 14 **Dong Y**, Wang WP, Mao F, Ji ZB, Huang BJ. Application of imaging fusion combining contrast-enhanced ultrasound and magnetic resonance imaging in detection of hepatic cellular carcinomas undetectable by conventional ultrasound. *J Gastroenterol Hepatol* 2016; **31**: 822-828 [PMID: 26480287 DOI: 10.1111/jgh.13202]
  - 15 **Xuan JW**, Bygrave M, Jiang H, Valiyeva F, Dunmore-Buyze J, Holdsworth DW, Izawa JJ, Bauman G, Moussa M, Winter SF, Greenberg NM, Chin JL, Drangova M, Fenster A, Lacefield JC. Functional neoangiogenesis imaging of genetically engineered mouse prostate cancer using three-dimensional power Doppler ultrasound. *Cancer Res* 2007; **67**: 2830-2839 [PMID: 17363606 DOI: 10.1158/0008-5472.CAN-06-3944]
  - 16 **Xing W**, Wang L, Maslov K, Wang LV. Integrated optical- and acoustic-resolution photoacoustic microscopy based on an optical fiber bundle. *Opt Lett* 2013; **38**: 52-54 [PMID: 23282835 DOI: 10.1364/OL.38.000052]
  - 17 **Yang JM**, Favazza C, Chen R, Yao J, Cai X, Maslov K, Zhou Q, Shung KK, Wang LV. Simultaneous functional photoacoustic and ultrasonic endoscopy of internal organs in vivo. *Nat Med* 2012; **18**: 1297-1302 [PMID: 22797808 DOI: 10.1038/nm.2823]

**P- Reviewer:** Goral V   **S- Editor:** Wang JL   **L- Editor:** Filipodia  
**E- Editor:** Huang Y





Published by **Baishideng Publishing Group Inc**  
7901 Stoneridge Drive, Suite 501, Pleasanton, CA 94588, USA  
Telephone: +1-925-223-8242  
Fax: +1-925-223-8243  
E-mail: [bpgoffice@wjgnet.com](mailto:bpgoffice@wjgnet.com)  
Help Desk: <http://www.f6publishing.com/helpdesk>  
<http://www.wjgnet.com>



ISSN 1007-9327

