

Supplementary Table 1 Subgroup analysis of the complete visualization rate and diagnostic yield of OMOM or MiroCam system

	OMOM system	MiroCam system	<i>P</i> value
The complete visualization rate (%)	72.4	78.8	0.169
The overall diagnostic yield (%)	57.2	60.8	0.497

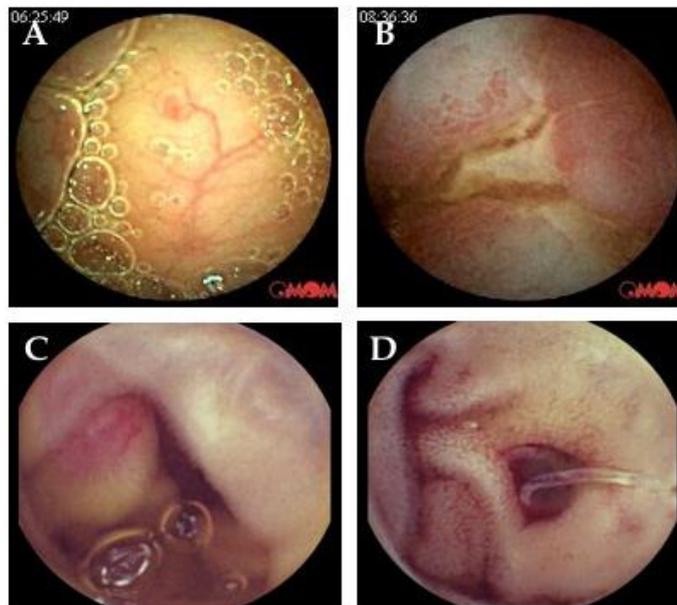


Figure1: A Angiodysplasia. B Crohn's disease. C Mass (gastrointestinal stromal tumors Confirmed by surgery). D Parasite.

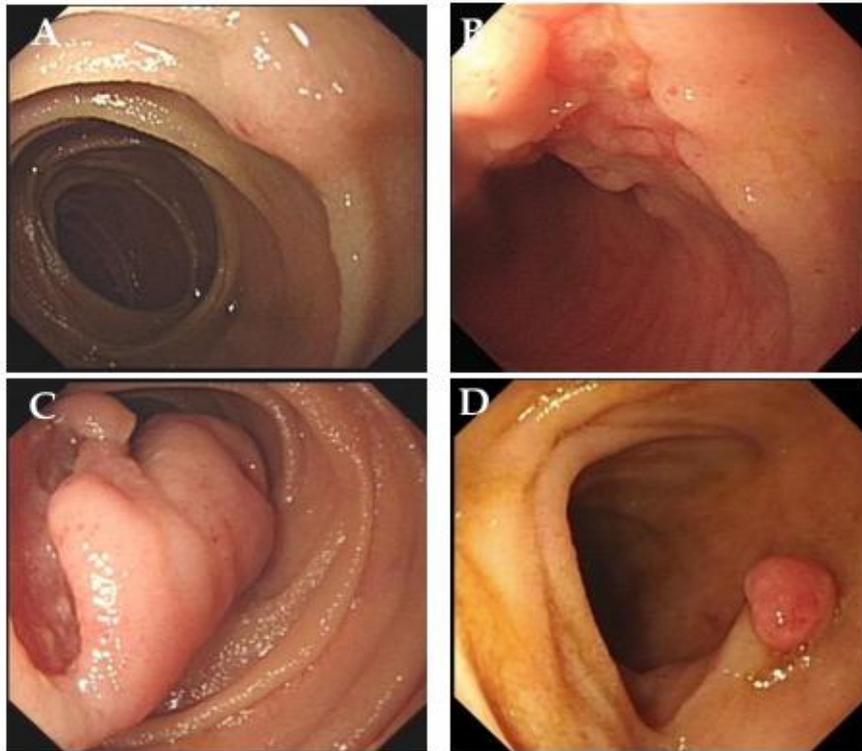


Figure2 : A Angiodysplasia. B Crohn's disease. C Mass (gastrointestinal stromal tumors Confirmed by surgery. D Polyp.